


FELLOW STAG EKG KETTLE

Guest User Manual for Fulham Pier Hotel

TURN ON

Push the main button to turn on your kettle.

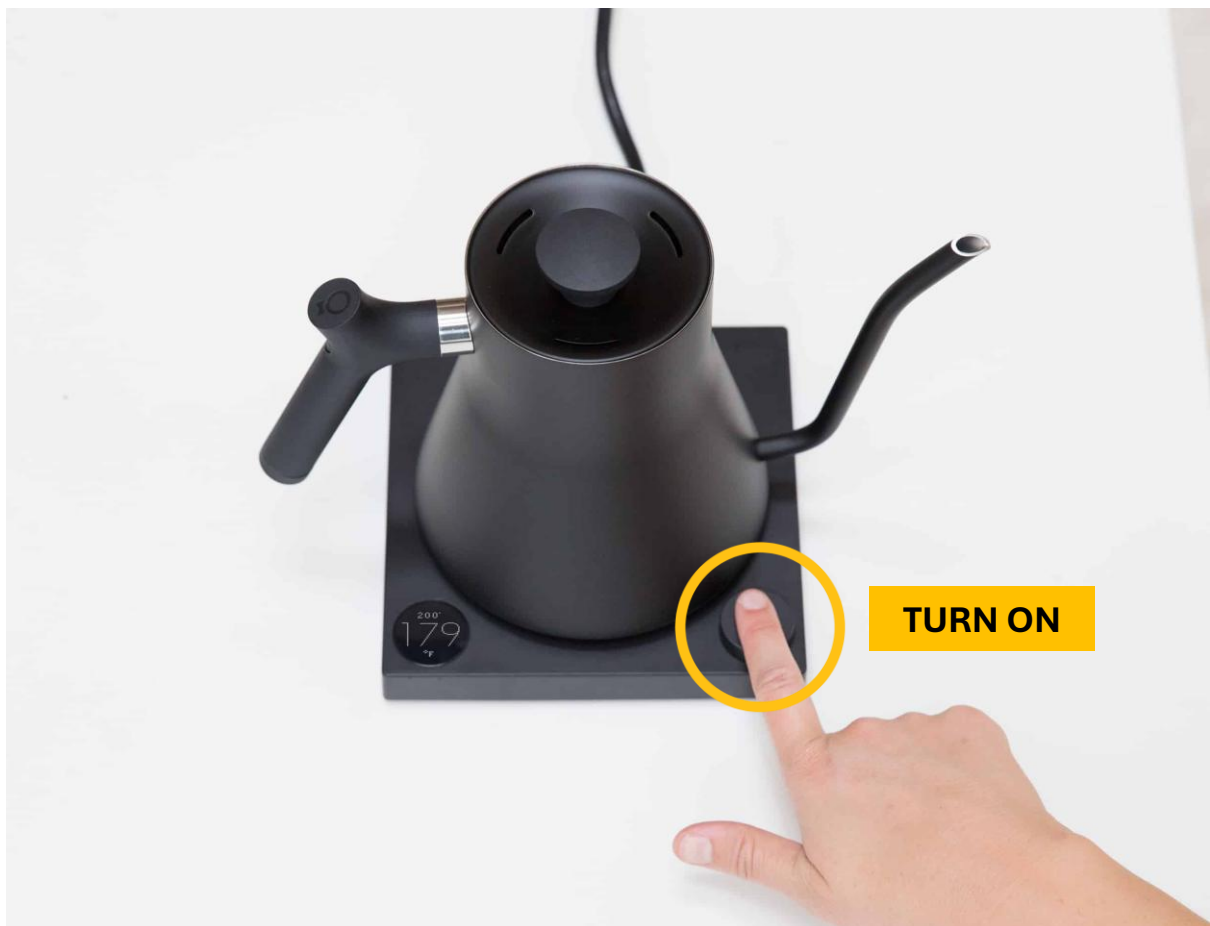

SET TEMPERATURE

Twist the main button to SET the desired temperature. The screen will show “SET” when the temperature is being set.



TEMPERATURE AND HOLD SETTINGS

- Use the back toggles to select your preferred temperature and HOLD settings. For temperature options, choose between Celsius and Fahrenheit.
- When activated, Stagg EKG's HOLD mode maintains your SET temperature for up to 60 minutes.
- If HOLD mode is off, your kettle will heat to the SET temperature, stay there for 5 minutes, then stop heating and enter standby for 15 minutes before turning off.
- When you enable HOLD mode, the screen will flash "HOLD ON". When your kettle maintains your SET temperature, HOLD will appear at the top of the LCD screen.



START/STOP BREW STOPWATCH

To start and stop the built-in Brew Stopwatch, hold down the main button for 2 seconds. Push the main button again to stop the stopwatch and return to the main screen.

